

The cutaneous uptake of atmospheric oxygen contributes significantly to the oxygen supply of human dermis and epidermis

M. Stücker †, A. Struk *†, P. Altmeyer †, M. Herde †, H. Baumgärtl * and D. W. Lübbers *

* Max-Planck-Institute for Molecular Physiology, Otto Hahn Str. 11, D-44227 Dortmund and † Department of Dermatology, Ruhr-University Bochum, Gudrunstrasse 56, D-44791 Bochum, Germany

It has been known since 1851 that atmospheric oxygen is taken up by the human epidermis. The contribution to total respiration is negligible. Until now the significance for the local oxygen supply of the skin has remained unknown. With a newly developed sensor, the oxygen fluxoptode, it has become possible to make local measurements of the transcutaneous oxygen flux (tcJ_{O_2}). In this study the sensor was calibrated so that absolute values of tcJ_{O_2} could be reported. At rest, tcJ_{O_2} was determined on normal, humidified skin on the volar forearm of 20 volunteers of different age groups. In order to evaluate the contribution of the blood flow to the oxygen supply of the skin, tcJ_{O_2} was recorded at the end of a 5 min suprasystolic occlusion of the forearm. At normal skin surface partial oxygen pressure (163 ± 9 Torr), tcJ_{O_2} was 0.53 ± 0.27 ml O_2 $min^{-1} m^{-2}$. A 5 min interruption of blood flow resulted in an increase of 9.5 ± 6.3 % in tcJ_{O_2} . The value of tcJ_{O_2} was unaffected by the age of the subject. Published data on the oxygen diffusion properties of skin and simulations of intracutaneous profiles of oxygen partial pressure indicated that under these conditions, the upper skin layers to a depth of 0.25–0.40 mm are almost exclusively supplied by external oxygen, whereas the oxygen transport of the blood has a minor influence. As a consequence, a malfunction in capillary oxygen transport cannot be the initiator of the development of superficial skin defects such as those observed in chronic venous incompetence and peripheral arterial occlusive disease.

(Resubmitted 23 July 2001; accepted after revision 19 October 2001)

Corresponding author M. Stücker: Department of Dermatology, Ruhr-University Bochum, Gudrunstrasse 56, D-44791 Bochum, Germany. Email: m.stuecker@derma.de

The skin is the only organ besides the lungs that is directly exposed to atmospheric oxygen. Apart from the stratum corneum, oxygen is consumed in all layers of the epidermis and dermis. The oxygen demand is partially satisfied by the blood: the dermis exhibits a vasculature that is arranged in two tiers that are parallel to the skin surface. The superficial plexus between the papillary and the upper reticular dermis deep plexus in the lower reticular dermis are connected by perpendicularly orientated communicating vessels. Arcades of capillaries loop upwards into the papillae from the subpapillary plexus (Braverman, 1989). In contrast, the epidermis has no vasculature, but is exposed directly to the atmosphere. As early as 1851, Gerlach was able to show that human skin takes up oxygen from the atmosphere.

Local relative measurements of the changes in cutaneous oxygen uptake from the atmosphere, the so-called transcutaneous oxygen flux (tcJ_{O_2}), have become possible with the development of an oxygen fluxoptode (Holst, 1994; Holst *et al.* 1995). Measurements of tcJ_{O_2} on the humidified skin of the volar forearm at normal skin temperature (33 °C) during artificially induced variations

in blood perfusion have indicated the functional relevance of the external oxygen supply (Stücker *et al.* 2000a). The induction of hyperaemia in moist skin with a combination of nonivamide and nicoboxil resulted in a distinct decrease of tcJ_{O_2} to 70 % of the resting values. These experiments clearly demonstrated that the oxygen supply of the corium is a balance between oxygen transport by the blood and uptake from the atmosphere. If the oxygen supply from the blood increases, a lower tcJ_{O_2} suffices to cover the oxygen demand of the skin. Stopping capillary oxygen transport was compensated by an increase of tcJ_{O_2} of only 9 %. This indicates that under normal conditions a substantial part of the upper skin is supplied by direct oxygen uptake from the atmosphere. Until now it has not been possible to determine the thickness of the layer (T) that characterises the contribution of tcJ_{O_2} to the total skin oxygen supply.

In a theoretical analysis, Fitzgerald (1957) estimated a mean T of 48 μm , with a range of 34–84 μm , which would cover the main part or the whole of the epidermis. His calculations were based on data for the diffusion coefficient measured on the anterior abdominal wall of the

frog following removal of the skin, because there were no comparable measurements on mammals. In fact, the true values for the oxygen permeability of skin tissue are an order of magnitude greater, whilst the oxygen consumption under normal conditions is about four times lower (actual data: 1470–2110 ml O₂ m⁻³ min⁻¹; Fitzgerald used 7800 ml O₂ (ml tissue)⁻¹ min⁻¹). The approximate partial pressure of oxygen (P_{O_2}) of capillary blood, 95 Torr (1 Torr = 0.1333 kPa), was taken as the minimum P_{O_2} of the skin. This is higher than the minimum value of 51 Torr that was measured in the skin *in vivo* using needle electrodes (Evans & Naylor, 1966a; Roszinski & Schmeller, 1995). A greater penetration depth T of the external oxygen is calculated using the latter values. Furthermore, Fitzgerald had to use data for the absorption of oxygen through the skin surface, which had a wide range of 0.4–2.9 ml O₂ m⁻² min⁻¹. This was due to different measuring locations and temperatures, large measuring areas and poor sensitivity of the measuring devices (for example, changes in the oxygen absorption caused by increased or decreased blood flow could not be detected).

In 1987, Baumgärtl *et al.* measured the intracutaneous profile of P_{O_2} directly with needle electrodes. The skin surface of the lower limb was covered by a film of water, which resulted in a reduced skin surface P_{O_2} of 78 Torr. Furthermore, the needle puncture probably produced a local hyperaemia and increased the oxygen supply by the blood. Under these conditions, with reduced skin surface P_{O_2} and hyperaemia, the P_{O_2} profile had a distinct minimum at a depth of about 100 μm , roughly at the level of the capillary loops (Fig. 1). These invasive measurements demonstrated a penetration depth of atmospheric oxygen

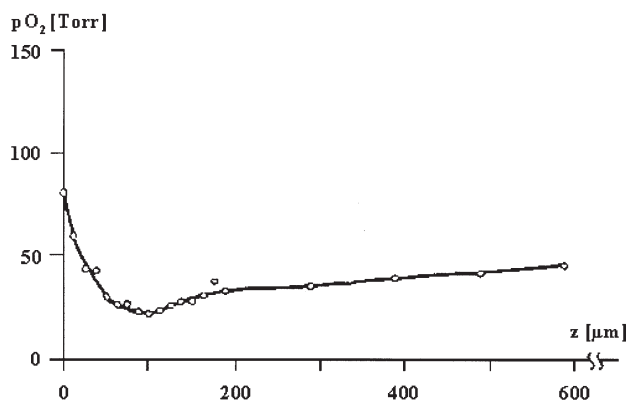


Figure 1. Oxygen partial pressure (P_{O_2}) measured by a needle electrode inserted perpendicularly into the skin

The depth z of the electrode is given in μm (skin surface at 0 μm). The skin surface was covered by a water film, resulting in a reduced skin surface P_{O_2} (ssP_{O_2}) of 78 Torr. The P_{O_2} profile has a distinct minimum at a depth of approximately 100 μm , roughly at the level of the dermo-epidermal junction (according to Baumgärtl *et al.* 1987). The needle puncture probably resulted in a local hyperemia. Under more physiological conditions, it is expected that the minimum would occur at a greater depth.

into the skin, double that of Fitzpatrick's estimated values. According to Fick's law of diffusion:

$$J_{O_2} = -K(\partial P_{O_2}/\partial x),$$

where J_{O_2} is the oxygen flux, K the conductivity and $\partial P_{O_2}/\partial x$ the pressure gradient. These measurements show, therefore, that in the upper 100 μm at least, there can only be a diffusion of oxygen from the skin surface to that depth instead of from the blood to the skin surface.

In this study, we have examined the importance of the cutaneous uptake of external oxygen for the skin supply by quantifying tcJ_{O_2} at a normal atmospheric P_{O_2} using a new, highly sensitive, non-invasive measuring device, which only covers small homogeneous skin areas rather than the large, heterogeneous skin areas with varying skin thicknesses and different densities of skin adnexes of earlier studies. In contrast to these earlier studies, it has been possible on the one hand to quantify absolute values (rather than relative changes in oxygen) by using a newly developed calibration system and, on the other, to measure at a normal instead of reduced skin surface P_{O_2} (Stücker *et al.* 2000a).

METHODS

Measurement of tcJ_{O_2}

Measurements were carried out using an oxygen fluxoptode developed by our group (Holst, 1994; Holst *et al.* 1995). This device consists of three different layers in a sandwich arrangement (Fig. 2). The fluxoptode is applied to the skin surface and represents an artificial barrier to the external atmosphere. The upper polymer layer serves as a diffusion barrier with a defined oxygen conductivity, whilst the oxygen-sensing silicon layer (with a negligible oxygen conductivity) allows measurement of the skin surface P_{O_2} (ssP_{O_2}). ssP_{O_2} is lower than the external atmospheric value as a result of the decreased oxygen flux (J_{O_2}) through the diffusion barrier. By increasing the external P_{O_2} , ssP_{O_2} can be varied until a stable value close to the normal atmospheric pressure is reached (Fig. 3C). At a given oxygen permeability P , the pressure difference (ΔP_{O_2}) between ssP_{O_2} and the external P_{O_2} is proportional to tcJ_{O_2} :

$$tcJ_{O_2} = \Delta P_{O_2} P. \quad (1)$$

It is thus possible to obtain an absolute value for tcJ_{O_2} if the oxygen permeability P of the diffusion barrier is known.

Oxygen fluxoptode

In order to obtain constant diffusion properties, the oxygen fluxoptodes were produced in our laboratory according to a standardised protocol. A commercially available polymer membrane (PFA 6510, Nowofol, Siegsdorf, Germany) with a thickness $d = 55 \mu\text{m}$ was used as the diffusion barrier. The value of P of this layer is given by:

$$P = K/d = \alpha D/d, \quad (2)$$

where K is the oxygen conductivity, α is the oxygen solubility and D is the oxygen diffusion constant.

ssP_{O_2} was measured optically using the oxygen indicator RuBiPy (Tris (2,2-bipyridyl) ruthenium (II) chloride hexahydrate; Strem

Chemicals, Kehl, Germany) adsorbed onto silica gel particles, which were embedded in a silicone layer with a high oxygen conductivity (Wacker Chemie, Burghausen, Germany). A further, blackened silicone layer in direct contact with the skin served as optical insulation to suppress fluorescence artefacts from the skin (Fig. 2). The measuring principle is based on the reduction of the fluorescence lifetime (quenching) of the indicator by oxygen. If the indicator is excited harmonically, the phase shift ($\Delta\Phi$) between excitation and fluorescence intensity is a measure of the oxygen concentration at the indicator molecules. The calibration curve is non-linear and is described by eqn (3) (Holst, 1994):

$$\Delta\Phi = A \frac{1 + CP_{O_2}}{1 + BP_{O_2}} \quad (3)$$

The oxygen fluxoptode was calibrated daily by exposing the fluxoptode to water-saturated N_2 - O_2 gas mixtures, the oxygen content of which varied from 0 to 20.95%. The parameters A , B and C were determined by a least squares fit (SigmaPlot 2.01, Jandel Scientific, Erkrath, Germany). The *in vitro* accuracy of the determination of ΔP_{O_2} was better than ± 0.2 Torr. A reproducibility of 5 Torr was obtained under our experimental conditions (Stücker *et al.* 2000a). The exponential equilibration time after changing the composition of the gas mixture was 87.9 ± 3.4 s ($n = 8$). No dependence on the oxygen concentration was observed. This value represents an upper limit, as the equilibration time was probably determined by the time course of the gas exchange within the volume of the calibration set-up.

Calibration of the oxygen fluxoptode and absolute determination of tcJ_{O_2}

The oxygen permeability of the diffusion barrier was determined using a polarographic oxygen electrode constructed according to the principles described by Lübbers *et al.* (1969). In this case, a large circular platinum cathode (\varnothing 1 mm) and an annular Ag-AgCl anode were used. The surface of the electrode was protected mechanically by a cellophane membrane (Bamberger, Wuppertal, Germany; thickness 25 μm) with high oxygen permeability. The membrane to be tested was placed in close contact with the cellophane membrane and exposed to the air. At an appropriate electrode potential (600–750 mV), all oxygen molecules crossing the membrane and reaching the platinum surface of the electrode are reduced, transferring four electrons per molecule (Aiba *et al.* 1968). The resulting current (I) at atmospheric oxygen pressure ($P_{O_2, \text{ATM}}$) is:

$$I = 4AP_{O_2, \text{ATM}}FK_{\text{TOTAL}} \quad (4)$$

where F is the Faraday constant and A is the electrode surface area (0.785 mm²). K_{TOTAL} is the combined oxygen permeability of the cellophane and the membrane to be tested. The oxygen permeability of the fluxoptode membrane was obtained by measuring the permeability of the cellophane membrane separately.

Seven fluxoptode membranes were tested for the 20 investigations in this study. The mean oxygen conductivity of the diffusion barrier was $K = 3.58 \pm 0.14 \times 10^{-7}$ ml O_2 min⁻¹ m⁻¹ Torr⁻¹. The thickness of the diffusion barrier for six of the optodes was 55 μm , with a tolerance of 1 μm . One membrane was exactly twice as thick, and although this led to a decreased permeability of the membrane, the transcutaneous oxygen uptake was unchanged compared to the other membranes.

Covering the electrode with the silicone layer of the fluxoptode resulted in no measurable decrease in the polarographic current.

This shows that this layer had no significant influence on the steady-state measurements of tcJ_{O_2} .

Skin humidity

The skin humidity was quantified using a corneometer SM 825 PC (Courage & Khazaka, Cologne, Germany). This uses the dielectric constant as a measure of the water content of the skin tissue. The measuring depth is approximately 15 μm .

Skin perfusion

The time course of the perfusion during the experiment and the efficacy of a suprasystolic occlusion were assessed by monitoring the transcutaneous P_{O_2} (tcP_{O_2} ; TCM 3, Radiometer, Copenhagen, Denmark) and the laser Doppler flow (DRT 4, Moor Instruments, Axminster, UK). The tcP_{O_2} and the laser Doppler sensor heads were positioned at a maximum distance of 10 mm from the fluxoptode. tcP_{O_2} was recorded at a skin temperature of 37°C (Huch *et al.* 1981) and laser Doppler flow at normal skin temperature (31–34°C) using a wavelength of 780 nm.

Subjects

Measurements were carried out on the volar forearm of 20 volunteers who had no clinical history or physical evidence on examination of vascular diseases, diabetes mellitus or skin diseases in the area examined. In order to evaluate whether tcJ_{O_2} is influenced by age, the group comprised two subgroups with 10 volunteers younger than 30 years (23.7 ± 3.1 years, 6 females, 4 males) and 10 volunteers older than 70 years (77.8 ± 5.4 years, 7 females, 3 males). Informed consent to participate was obtained from all of the subjects. A histological examination was carried out on one subject for diagnostic reasons unrelated to this study. The study protocol was reviewed and approved by the Ethics Committee of Ruhr University, Bochum, and was carried out in accordance with the Helsinki guidelines.

Experimental design

The volunteers were acclimatised at a room temperature of 22–23°C for 20–25 min lying in a comfortable supine position with the upper body slightly raised. Before applying the probe, the skin in the test area was cleaned with 63% propanol (Cutasept, Bode Chemie, Hamburg, Germany). The superficial horny scales were removed by stripping 10 times with adhesive tape. Sejrnsen (1968) demonstrated that the removal of the outer stratum

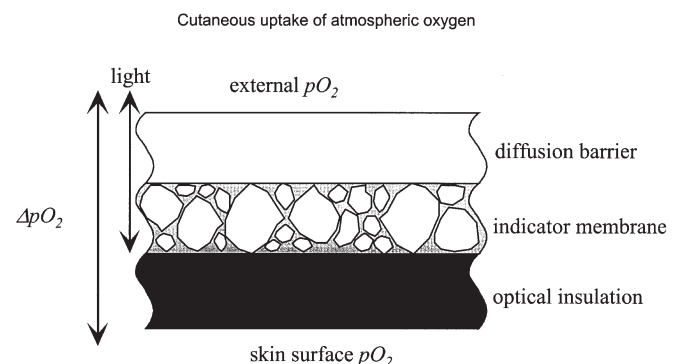


Figure 2. Cross section of the oxygen fluxoptode (according to Holst, 1994)

The oxygen flux through the diffusion barrier induces a pressure gradient, ΔP_{O_2} . The P_{O_2} in the highly oxygen-permeable indicator membrane is measured with an optical oxygen indicator adsorbed onto silica gel particles. The external P_{O_2} can be varied to adjust the ssP_{O_2} close to the atmospheric value ('normobaric conditions').

disjunctum of the horny layer had no effect on the diffusion of xenon, but that by removing the stratum conjunctum and stratum granulosum (stripping 40–50 times), diffusion increased up to 40 times (skin temperature 33 °C at room temperature). At the beginning and end of the measurement, the tcJ_{O_2} sensor signal was recorded at normal atmospheric P_{O_2} as a reference value. After humidifying the skin in the test area with 50 μ l water, the measuring heads were fixed in position with adhesive rings. The temperature of the sensor heads was adjusted to 33 °C.

Figure 3 shows a typical example of the course of the tcJ_{O_2} measurement. In order to characterise the influence of changes of the skin perfusion on tcJ_{O_2} at normal ssP_{O_2} a 5 min suprasystolic occlusion was carried out with a blood pressure cuff applied to the upper arm.

The skin humidity was measured at the start, after the stripping procedure and at the end of the measurement period. To differentiate between the changes in skin humidity due to the measuring procedure and those due to normal physiological alterations, corneometric measurements were also carried out on untreated skin in close proximity to the test area.

Statistics

Data are presented as means \pm s.d. The data were tested for Gaussian distribution with the Kolmogorov-Smirnov test. The significance of any differences was tested with the t test (SPSS 8.0, SPSS, Chicago, IL, USA). The significance level was set at $P = 0.05$.

RESULTS

Case example

Figure 3 shows a typical course of a tcJ_{O_2} measurement. Within 16 min of applying the sensor to the volar forearm (A), the ssP_{O_2} decreased from the normal atmospheric

value to a steady-state value of 75 Torr (B), corresponding to a pressure difference across the diffusion barrier (ΔP_{O_2}) of 85 Torr.

After application of the oxygen fluxoptode, ssP_{O_2} equilibrated exponentially during the period defined by a change in ΔP_{O_2} from 75 to 100 % of the final value. In this case, an exponential fit revealed an equilibration time (τ) of 244 s, which is within the range of data published previously (Stücker *et al.* 2000a).

Increasing the external P_{O_2} to 314 Torr resulted in an ssP_{O_2} close to the atmospheric value (C, 'normobaric conditions'). At this point, ΔP_{O_2} was 154 Torr.

In order to examine the influence of an interruption of the blood supply under normobaric conditions, a suprasystolic occlusion was carried out for 5 min while the external P_{O_2} of 314 Torr remained constant (D).

There was a considerable time lapse between the change of the external P_{O_2} and the equilibration of the ssP_{O_2} to the new steady state due to the equilibration time of the fluxoptode. It was usually not possible to wait until the signal was totally stable, and the steady-state value was therefore determined by subtracting a linear baseline (D, dotted line). In this experiment, a decrease in the ssP_{O_2} of 3.3 Torr was observed at the end of the occlusion.

The oxygen permeability of the fluxoptode was 6.36×10^{-3} ml O_2 m^{-2} min^{-1} Torr $^{-1}$, yielding a tcJ_{O_2} of

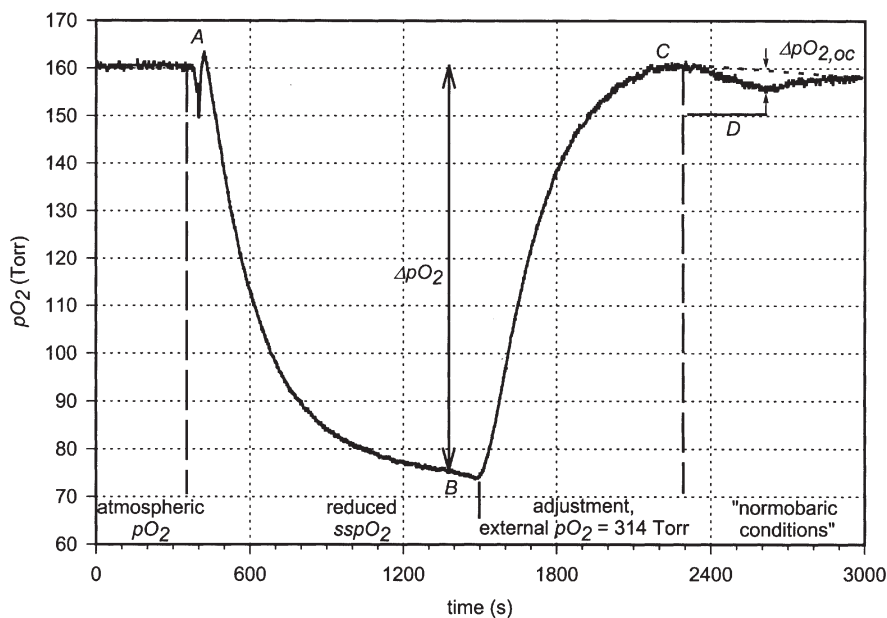


Figure 3. Case example of a measurement of the transcutaneous oxygen flux (tcJ_{O_2} ; 24-year-old female volunteer, no. 6)

The normal atmospheric P_{O_2} was recorded between 0 and 400 s. At A, the oxygen fluxoptode was applied to the volar forearm. ssP_{O_2} reached a steady level at B, indicating a ΔP_{O_2} of 85 Torr (equilibration time). Between points B and C, the external P_{O_2} was increased to 314 Torr to adjust the ssP_{O_2} to 'normal atmospheric conditions'. In the time interval D, a suprasystolic occlusion was carried out, resulting in an increase in ΔP_{O_2} ; ΔP_{O_2} during occlusion ($\Delta P_{O_2,oc}$) = 3.3 Torr. $\Delta P_{O_2,oc}$ was determined by subtraction of a linear baseline (dotted line).

Table 1. Measurements of transcutaneous oxygen flux (tcJ_{O_2} ; 33 °C, humidified skin)

Volunteer	Age (years)	No pressure correction		Normal ssp_{O_2}		Occlusion ΔtcJ_{O_2} (ml O ₂ min ⁻¹ m ⁻²)
		ssp_{O_2} (Torr)	tcJ_{O_2} (ml O ₂ min ⁻¹ m ⁻²)	ssp_{O_2} (Torr)	tcJ_{O_2} (ml O ₂ min ⁻¹ m ⁻²)	
1	22	99	0.38	164	0.54	0.020
2	23	110	0.31	159	0.34	0.046
3	23	97	0.39	156	0.47	0.036
4	25	112	0.29	159.5	0.45	0.041
5	20	99	0.38	152	0.69	0.056
6	24	75	0.54	160	0.98	0.021
7	28	104	0.19	172	0.24	0.047
8	19	97	0.21	168	0.30	0.046
9	29	84	0.26	163	0.43	0.034
10	24	102	0.37	160	0.71	0.026
11	79	94	0.42	160	0.65	0.045
12	81	99	0.38	156	0.71	0.019
13	70	116	0.28	172	0.33	0.032
14	77	104	0.35	156	0.35	0.060
15	81	96	0.40	166	0.70	0.050
16	79	99	0.41	185	0.72	0.028
17	84	109	0.31	164	0.59	0.038
18	70	91	0.46	148	1.13	0.034
19	83	134	0.16	176	0.07	0.016
20	70	106	0.18	166	0.18	0.035
Mean		101.4	0.334	163	0.529	0.037
s.d.		12.2	0.100	9	0.265	0.013

tcJ_{O_2} is significantly reduced at lower values of skin surface partial pressures of oxygen (P_{O_2}).

0.54 ml O₂ m⁻² min⁻¹ at the lower ssp_{O_2} and 0.98 ml O₂ m⁻² min⁻¹ under normobaric conditions at the skin surface. The increase in the tcJ_{O_2} induced by the occlusion was 0.021 ml O₂ m⁻² min⁻¹.

Measurement of tcJ_{O_2} under normobaric conditions

After appropriate variation of the external P_{O_2} , an average ssp_{O_2} of 163 ± 9 Torr was reached. The ΔP_{O_2} across the membrane of 90 ± 37 Torr was measured (Table 1) under these conditions.

After determination of the oxygen permeability of the fluxoptode, the transcutaneous oxygen uptake could be calculated using eqn (1). tcJ_{O_2} was found to be 0.529 ± 0.265 ml O₂ m⁻² min⁻¹ (Fig. 4).

Interruption of the blood supply

In this study the effect of an interruption of blood flow (ischaemia) was evaluated under normobaric conditions. On average, the laser Doppler flow decreased from 21.0 ± 7.8 arbitrary units (a.u.) to 5.0 ± 1.5 a.u. ($P \leq 0.0001$). During the post-occlusional reactive hyperaemia it increased by 305 ± 165 % within 40.6 ± 52.2 s, followed by a decay to the baseline value ($P \leq 0.0001$). The tcP_{O_2} values were 7.1 ± 7.3 Torr at rest and 1.6 ± 2.4 Torr during suprasystolic occlusion ($P \leq 0.0001$). The post-reactive hyperaemia represented a relative increase of 372 ± 336 % compared to the resting values ($P \leq 0.0001$).

At the end of the 5 min suprasystolic occlusion the ssp_{O_2} below the oxygen fluxoptode was decreased by 6.8 ± 3.3 Torr (measured as the distance to a linear baseline; C in Fig. 3, $P \leq 0.0001$). This value indicates a mean increase in tcJ_{O_2} of 0.037 ± 0.013 ml O₂ m⁻² min⁻¹. The occlusion resulted in a relative elevation of tcJ_{O_2} of 9.5 ± 6.3 % ($P \leq 0.05$, Fig. 4).

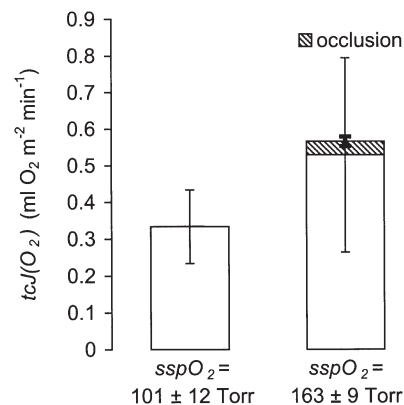


Figure 4. Comparison of the tcJ_{O_2} (33 °C, humidified skin) under normal (right) and reduced (left) ssp_{O_2} ($n = 20$)

A 5 min suprasystolic occlusion resulted in only a small increase (shaded area).

The tcJ_{O_2} at a lower ssP_{O_2}

tcJ_{O_2} produced a decrease of ssP_{O_2} below the oxygen fluxoptode to 101.4 ± 12.2 Torr (Fig. 4, left). These data correspond to a ΔP_{O_2} across the diffusion barrier of 60.0 ± 11.9 Torr. This is equivalent to a tcJ_{O_2} of 0.334 ± 0.100 ml O_2 m^{-2} min^{-1} , representing $68 \pm 17\%$ of the values determined under normobaric conditions (Fig. 4, right).

A mono-exponential equilibration time, τ , was found in 17 experiments. A multi-exponential time dependence was found in three experiments. These measurements were omitted because it was suggested that in these cases there was not an adequate airtight seal between the sensor and the skin surface. The mean exponential equilibration time was 413 ± 130 s.

Dependence on age

There was no significant difference in tcJ_{O_2} between the subgroups of young and old volunteers. Under normobaric conditions, tcJ_{O_2} was 0.515 ± 0.224 ml O_2 m^{-2} min^{-1} (young volunteers) and 0.543 ± 0.313 ml O_2 m^{-2} min^{-1} (old volunteers; $P = 0.83$). The relative increase during a suprasystolic occlusion was $9.1 \pm 5.6\%$ and $9.9 \pm 7.3\%$, in the young and old subjects, respectively ($P = 0.80$).

Changes in the skin humidity

On average, at the beginning of the measurements the mean value of the skin humidity of untreated skin was 43 ± 11 a.u. (Fig. 5). After stripping the skin 10 times with adhesive tape, the skin humidity increased significantly to 49 ± 13 a.u. ($P \leq 0.0001$). A value of 78 ± 24 a.u. was recorded at the end of the measurements, after removal of the oxygen fluxoptode. The humidity of untreated skin close to the test area was 63 ± 16 a.u. at this time. These numbers represent a relative increase of $86 \pm 61\%$ in the test area and $51 \pm 42\%$ in the reference area ($P \leq 0.0032$).

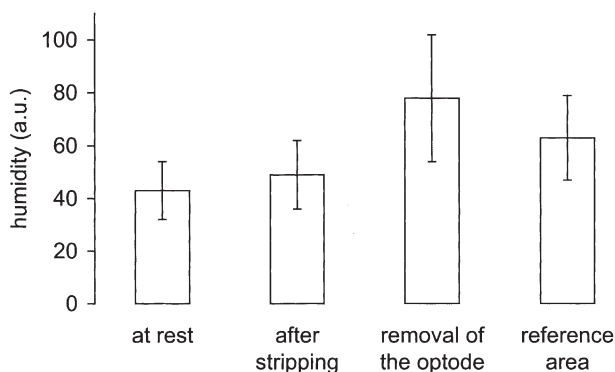


Figure 5. Change of skin humidity during the investigations (n = 20)

The skin humidity is given in arbitrary units (a.u.). An increase of humidity in the measurement area resulted from the stripping procedure and from the sealing of the skin surface by the oxygen fluxoptode. Measurements in the reference area showed a parallel increase of the humidity of untreated skin.

DISCUSSION

Contribution of tcJ_{O_2} to the oxygen supply of the whole organism

The transcutaneous oxygen uptake of 0.529 ± 0.265 ml O_2 m^{-2} min^{-1} , as determined in this study, is at the lower end of the wide range of 0.4 – 2.9 ml O_2 m^{-2} min^{-1} quoted in the literature (see Fitzgerald, 1957). Assuming a body surface area of 1.7 m^2 , this yields a total transcutaneous oxygen uptake of 0.90 ± 0.45 ml O_2 m^{-2} min^{-1} , which represents only 0.4% of the pulmonary oxygen uptake at rest (*ca* 230 ml O_2 min^{-1} ; see Wade & Bishop, 1962). The contribution of tcJ_{O_2} to the oxygen supply of the whole organism is therefore negligible under normal conditions.

Estimation of the skin tissue supplied by tcJ_{O_2}

The thickness of the skin tissue (T) that is supplied by external oxygen can be estimated if the whole amount of oxygen taken up from the atmosphere is consumed within the skin. Since in all the experiments in this study an increase of tcJ_{O_2} was observed during ischaemia, capillary oxygen removal from the skin is negligible. Furthermore, assuming a homogeneous oxygen consumption (\dot{V}_{O_2}) in the upper skin layers, T is given by:

$$T = tcJ_{O_2} / \dot{V}_{O_2} \quad (5)$$

\dot{V}_{O_2} in skin tissue has been investigated *in vivo* by determination of the decrease in P_{O_2} after stopping the oxygen supply. It was found to be strongly temperature dependent. At 43 $^{\circ}C$ $\dot{V}_{O_2} = 4700$ ml O_2 m^{-3} min^{-1} was derived from tcP_{O_2} measurements (Severinghaus *et al.* 1978; Stücker *et al.* 2000b). At about 35 $^{\circ}C$, a oxygen uptake value of 1470 ml O_2 m^{-3} min^{-1} has been measured with intradermal needle electrodes (Evans & Naylor, 1966b), whereas measurements on the stratum papillare without epidermis revealed a \dot{V}_{O_2} of 2110 ml O_2 m^{-3} min^{-1} (blister base, Evans & Naylor, 1967). On the surface of the epidermis (blister lid) it was found to be 1990 ml O_2 m^{-3} min^{-1} (Evans & Naylor, 1967).

With values between 1470 and 2110 ml O_2 m^{-3} min^{-1} , eqn (5) yields $T = 251$ – 360 μm . Since there is no oxygen consumption in the stratum corneum with a typical thickness of 15 μm , the total thickness of the skin supplied by external oxygen can be estimated to be 266 – 375 μm .

Comparison with a theoretical analysis

It is also possible to deduce tcJ_{O_2} and T from the diffusion properties of oxygen in skin tissue if the oxygen transport by blood is described by a model. Models examining the meaning of tcP_{O_2} have been published (see Huch *et al.* 1981; Grossmann, 1982; Lübbers, 1994), but a similar analysis of the tcJ_{O_2} is lacking. The following assumptions are used to calculate intracutaneous P_{O_2} profiles:

(1) Under normal conditions the upper skin layers are supplied exclusively by the diffusion of oxygen from the

atmosphere. This assumption is justified by the observation of only small changes of tcJ_{O_2} during occlusion.

(2) Experiments using polarographic P_{O_2} needle electrodes have revealed characteristics of the intracutaneous P_{O_2} profiles: the P_{O_2} decreases continuously from a maximum at the skin surface to the upper layers of the papillary dermis until reaching a minimum, followed by a slight increase in the deeper skin layers (Fig. 1, Baumgärtl *et al.* 1987). According to Fick's first law ($J_{O_2} = -K(\partial P_{O_2}/\partial x)$), there is no oxygen flux (J_{O_2}) between the upper layer where the P_{O_2} is decreasing and the skin tissue below the point at which the minimum is reached.

A mean intracutaneous P_{O_2} of 51 Torr has been recorded at greater depths (Evans & Naylor, 1966a; Roszinski & Schmeller, 1995). We assume, therefore, that there is an intracutaneous P_{O_2} minimum of 51 Torr. Its depth depends on the other parameters.

(3) The oxygen permeabilities (K) are 3.7×10^{-7} ml O_2 m^{-1} min^{-1} Torr $^{-1}$ in the stratum corneum and 1.3×10^{-6} ml O_2 m^{-1} min^{-1} Torr $^{-1}$ in viable tissue (measured at 32 °C; Grossmann, 1982; for an overview see Huch *et al.* 1981).

(4) As described above, a \dot{V}_{O_2} value of 1990 ml O_2 m^{-3} min^{-1} is assumed for the epidermis (Evans & Naylor, 1967) and 1470 ml O_2 m^{-3} min^{-1} for dermal tissue (Evans & Naylor, 1966b).

These assumptions allow an algebraic static solution of Fick's second law:

$$K(\partial^2 P_{O_2}/\partial x^2) = -(\partial c_{O_2}/\partial t) = \dot{V}_{O_2}, \quad (6)$$

where c_{O_2} is the concentration of dissolved oxygen). Equation (7) represents the general solution in a homogeneous tissue layer:

$$P_{O_2}(x) = (\dot{V}_{O_2}/2K)x^2 + c_1x + c_2, \quad (7)$$

with the integration constants c_1 and c_2 (x -axis perpendicular to the skin surface). The application of Fick's first law yields J_{O_2} at position x :

$$J_{O_2} = \dot{V}_{O_2}x + c_1, \quad (8)$$

c_1 and c_2 result from the boundary conditions of each skin layer, starting from the P_{O_2} minimum with $P_{O_2} = 51$ Torr and $J_{O_2} = 0$.

Trace A on Fig. 6 shows the P_{O_2} profile derived according to the described assumptions. The skin tissue is supplied with external oxygen to a depth of 403 μm . The calculated tcJ_{O_2} is 0.58 ml O_2 m^{-2} min^{-1} . This value is in agreement with the data obtained from our experiments (0.529 ± 0.265 ml O_2 m^{-2} min^{-1}), indicating that the model represents a good description of the oxygen transport in the upper skin layers.

Comparison with the experiments with needle electrodes

Baumgärtl *et al.* (1987) measured an intracutaneous P_{O_2} profile in the lower leg using a polarographic needle electrode. A water film at the skin surface reduced the ssP_{O_2} to 78 Torr. A minimum of $P_{O_2} = 22$ Torr was observed at a minimum depth of 100 μm . Adaptation of eqn (7) to this curve (with the minimum at $x = 0$) yields (Fitzgerald, 1957):

$$T_{min} = \sqrt{((2K/\dot{V}_{O_2})(ssP_{O_2} - P_{O_2,min}))}, \quad (9)$$

This allows the depth T , which would be observed under normobaric conditions under the assumption of an unaltered minimal pressure, to be calculated:

$$T = T_{min}\sqrt{((160 \text{ Torr} - P_{O_2,min})/(78 \text{ Torr} - P_{O_2,min}))}, \quad (10)$$

The resulting value of 188 μm is still distinctly lower than the other estimates. Although this investigation was carried out in the lower leg, the difference cannot be attributed to regional variations. The ΔP_{O_2} across the fluxoptode (measured without pressure correction) at the medial ankle (72.8 ± 12.3 Torr; Stücker *et al.* 2000a) is even greater than in the volar forearm (60.0 ± 11.9 Torr;

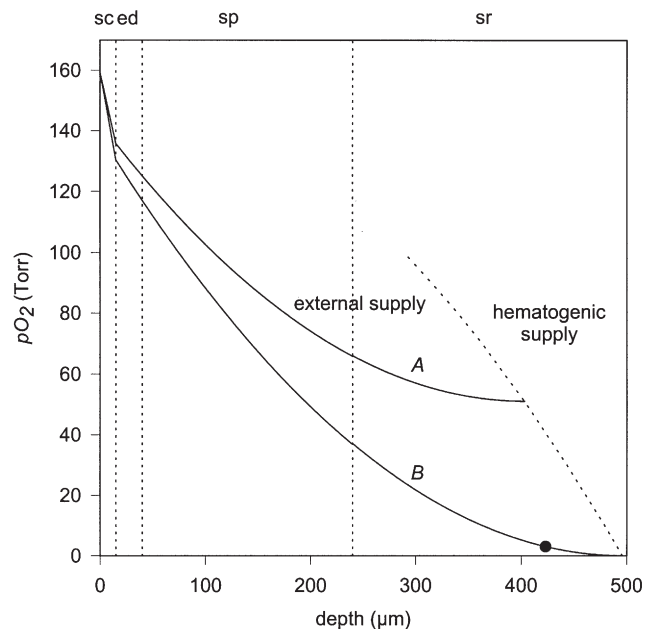


Figure 6. Theoretical estimation of the intracutaneous P_{O_2} profile

The P_{O_2} minimum at 51 Torr (trace A) and at 0 Torr (trace B: suprasystolic occlusion) are shown. Below a critical P_{O_2} of about 3 Torr, mitochondrial activity is reduced (Wilson, 1979). Skin surface at $x = 0$; sc: stratum corneum; ed: viable epidermis; sp: stratum papillare; sr: stratum reticulare. The area on the right side of the dotted line is supplied by blood. Temperature: 32 °C; oxygen permeabilities: 3.7×10^{-7} ml O_2 m^{-1} min^{-1} Torr $^{-1}$ (stratum corneum) and 1.3×10^{-6} ml O_2 m^{-1} min^{-1} Torr $^{-1}$ (viable layers); oxygen consumption = 1990 ml O_2 m^{-3} min^{-1} (viable epidermis) and 1470 ml O_2 m^{-3} min^{-1} (dermal tissue). ● = 3 Torr.

this study). The difference might be explained by tissue damage due to the needle puncture and consequential hyperaemia.

Figure 7 correlates the different estimates of T with skin morphology. It shows that the whole epidermis and parts of the dermis are supplied by external oxygen from the air.

Interruption of the blood supply

During a 5 min suprasystolic occlusion, tcJ_{O_2} increased by $0.037 \pm 0.013 \text{ ml O}_2 \text{ m}^{-2} \text{ min}^{-1}$, representing a relative increase of only $9.5 \pm 6.3\%$. The measurement of the tcP_{O_2} , representing the nutritive blood flow (Bongard & Bounameaux, 1993) proved the efficacy of this test: tcP_{O_2} decreased from 7.1 ± 7.3 Torr to 1.6 ± 2.4 Torr. Due to the equilibration time of the fluxoptode of 413 ± 130 s, ssP_{O_2} did not reach a stable equilibrium value during the

limited period of suprasystolic occlusion (300 s). A further reason for the non-attainment of a steady state of the ssP_{O_2} during the 5 min occlusion may be that the tissue oxygen saturation values did not approach a minimum value and therefore it is possible that not all the available oxygen had been unloaded from the haemoglobin within the microcirculation. As a consequence, the values of ΔtcJ_{O_2} determined may result in an underestimate of the contribution of oxygen by the blood. However, even the measurements with shorter equilibration times (e.g. the case example) showed only a minor increase in tcJ_{O_2} during suprasystolic occlusion. This indicates that in our measurements the capillary contribution to the oxygen supply of the corium is very limited.

In trace B of Fig. 6, a suprasystolic occlusion is simulated by assuming an intracutaneous P_{O_2} of 0 Torr in deeper skin

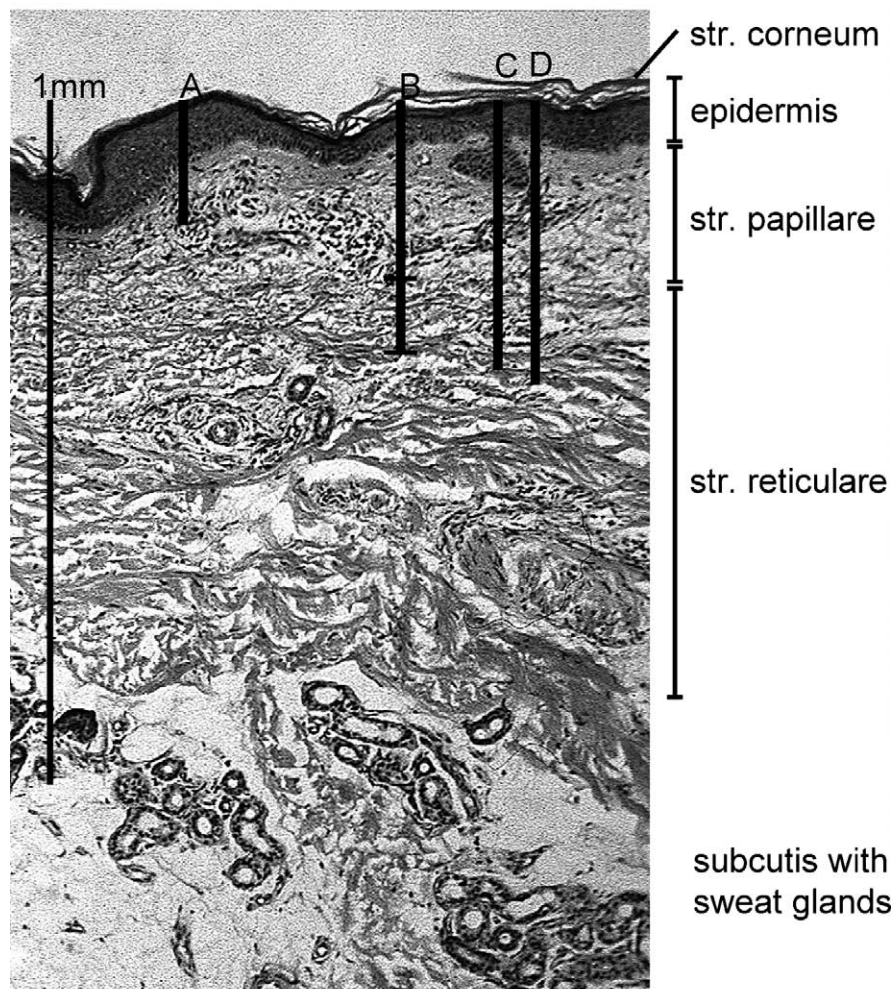


Figure 7. Penetration depth of atmospheric oxygen in the skin: different estimations

Histological section of healthy skin from the volar forearm (male subject, 64 years old) with different estimates of the thickness, T , of the skin layer that is supplied from the atmosphere. (Normal ssP_{O_2} , humid skin, skin temperature 33°C). A: $T = 188 \mu\text{m}$. Extrapolation from data obtained from invasive experiments with P_{O_2} needle electrodes (Baumgärtl *et al.* 1987). B: $T = 266\text{--}375 \mu\text{m}$. Estimation using the tcJ_{O_2} values determined in this study. C: $T = 403 \mu\text{m}$ and D: $T = 423 \mu\text{m}$. Estimation of T using published data for the oxygen diffusion properties and oxygen consumption in skin tissue, assuming an intradermal P_{O_2} of 51 Torr (C, normal conditions) and of 0 Torr (D, ischaemia).

layers. Under this condition, tcJ_{O_2} increased by 24%. Because this value was calculated assuming a steady-state situation, it agrees with the experimental data. Under the assumption of a minimal P_{O_2} of 3 Torr, which is necessary to maintain mitochondrial activity (Wilson *et al.* 1979), tcJ_{O_2} can cover the oxygen demand of the upper 423 μm of the skin if blood perfusion is interrupted.

tcJ_{O_2} under hypobaric conditions

Without pressure correction, tcJ_{O_2} produced a ΔP_{O_2} of 60 ± 12 Torr across the oxygen fluxoptode. This value is significantly lower than the previously published data. Using identical oxygen fluxoptodes, Stücker *et al.* (2000a) found values of 72.8 ± 12.3 Torr at the medial ankle and 81.8 ± 8.5 Torr on the abdomen. Such variations of tcJ_{O_2} could be the result of differences in the skin structure, skin perfusion or different adnex densities.

Skin humidity

The oxygen permeability of tissue is strongly dependent upon water content (Vaupel, 1976). During the investigations in this study, the humidity of the skin below the oxygen fluxoptode (measured with the Corneometer) increased significantly from 43 ± 11 a.u. to 78 ± 24 a.u. due to the stripping procedure, artificial humidification of the skin or just sweating. A lower J_{O_2} is to be expected through dry skin. Nevertheless, the skin humidity in the measurement area did not differ greatly from the normal physiological range, as was shown by the comparison with the untreated reference area where values of 63 ± 16 a.u. were observed.

Age dependence

Skin in elderly people displays characteristic functional and structural alterations such as changes in permeability to drugs (Malkinson, 1958) and increased corneocyte surface (Marks, 1981). Effects such as a reduction in thickness and cell density of the corium, keratoses and elastoses are clearly related to long-term UV exposure (Balin & Lin, 1989; Yaar & Gilchrist, 1999) and should be absent in the volar forearm. No influence on the transepidermal oxygen uptake was found due to intrinsic alterations in aged skin, since the tcJ_{O_2} at this location proved to be unaffected by age.

Clinical relevance

In this study it has been shown that under normal conditions, atmospheric oxygen can supply the upper skin layers to a depth of 0.25–0.40 mm. This is 3–10 times deeper than has been calculated previously (Fitzgerald, 1957; Baumgärtl *et al.* 1987). The whole epidermis and the upper corium can therefore be supplied with oxygen from the atmosphere. For the first time, all of the data have been derived from non-invasive measurements *in vivo* in human skin instead of *in vitro* measurements in non-mammalian skin (Fitzgerald, 1957) or single invasive measurements (Baumgärtl *et al.* 1987). This may have

significant consequences with regard to the treatment of lesions such as venous and ischaemic ulcers.

REFERENCES

- AIBA S., OHASHI, M. & HUANG, S. Y. (1968). Rapid determination of oxygen permeability of polymer membranes. *Industrial and Engineering Chemistry Fundamentals* **7**, 497–502.
- BALIN, A. K. & LIN, A. N. (1989). Skin changes as a biological marker for measuring the rate of human aging. In *Aging and the Skin*, ed. BALIN, A. K. & KLIGMAN, A. M., pp. 43–75. Raven, New York.
- BAUMGÄRTL, H., EHRLY, A. M., SAEBER-LORENZ, K. & LÜBBERS, D. W. (1987). Initial results of intracutaneous measurements of PO_2 profiles. In *Clinical Oxygen Pressure Measurement*, ed. EHRLY, A. M., HAUSS, J. & HUCH, R., pp. 121–128. Springer, Berlin.
- BONGARD, O. & BOUNAMEAUX, H. (1993). Clinical investigation of skin microcirculation. *Dermatology* **186**, 6–11.
- BRAVERMAN, I. M. (1989). Ultrastructure and organization of the cutaneous microvasculature in normal and pathologic states. *Journal of Investigative Dermatology* **93**, 2S–9S.
- EVANS, N. T. S. & NAYLOR, P. F. D. (1966a). Steady states of oxygen tension in human dermis. *Respiration Physiology* **2**, 46–60.
- EVANS, N. T. S. & NAYLOR, P. F. D. (1966b). The dynamics of changes in dermal oxygen tension. *Respiration Physiology* **2**, 61–72.
- EVANS, N. T. S. & NAYLOR, P. F. D. (1967). The oxygen tension gradient across human epidermis. *Respiration Physiology* **3**, 38–42.
- FITZGERALD, L. R. (1957). Cutaneous respiration in man. *Physiological Reviews* **37**, 325–345.
- GERLACH, A. (1851). Über das Hautathmen. *Archives of Anatomy and Physiology* 431–479.
- GROSSMANN, U. (1982). Simulation of combined transfer of oxygen and heat through the skin using a capillary-loop model. *Mathematical Biosciences* **61**, 205–236.
- HOLST, G. (1994). Entwicklung und Erprobung einer Sauerstoff-Flux-Optode mit einem Sauerstoff-Sensor nach dem Prinzip der dynamischen Fluoreszenzlöschung. Fortschritt-Berichte VDI Reihe 17 Nr. 111, pp. 1–105. VDI Verlag, Düsseldorf.
- HOLST, G., KÖSTER, T., VOGES, E. & LÜBBERS, D. W. (1995). FLOX—an oxygen-flux-measuring system using a phase-modulation method to evaluate the oxygen-dependent fluorescence lifetime. *Sensors and Actuators B* **29**, 231–239.
- HUCH, R., HUCH, A. & LÜBBERS, D. W. (1981). *Transcutaneous PO_2* . Thieme-Stratton, New York.
- LÜBBERS, D. W. (1994). Microcirculation and O_2 exchange through the skin surface. A theoretical analysis. *Advances in Experimental Medicine and Biology* **361**, 51–58.
- LÜBBERS, D. W., BAUMGÄRTL, H., FABEL, H., HUCH, A., KESSLER, M., KUNZE, K., RIEMANN, H., SEILER, D. & SCHUCHHARDT, S. (1969). Principle of construction and application of various platinum electrodes. *Progress in Respiration Research* **3**, 136–146.
- MALKINSON, F. D. (1958). Studies on percutaneous absorption of ^{14}C labelled steroid by use of the gas flow cell. *Journal of Investigative Dermatology* **31**, 19–28.
- MARKS, R. (1981). Measurement of biological aging in human epidermis. *British Journal of Dermatology* **104**, 627–633.
- ROSZINSKI, S. & SCHMELLER, W. (1995). Differences between intracutaneous and transcutaneous skin oxygen tension in chronic venous insufficiency. *Journal of Cardiovascular Surgery* **36**, 407–413.
- SEJRSEN, P. (1968). Epidermal diffusion barrier to ^{133}Xe in man and studies of clearance of ^{133}Xe by sweat. *Journal of Applied Physiology* **24**, 211–216.

- SEVERINGHAUS, J. W., STAFFORD, M. & THUNSTROM, A. M. (1978). Estimation of skin metabolism and blood flow with tcpO₂ and tcpCO₂ electrodes by cuff occlusion of the circulation. *Acta Anaesthesiologica Scandinavica. Supplementum* **68**, 9–15.
- STÜCKER, M., ALTMAYER, P., STRUK, A., HOFFMANN, K., SCHULZE, L., RÖCHLING, A. & LÜBBERS, D. W. (2000a). The transepidermal oxygen flux from the environment is in balance with the capillary oxygen supply. *Journal of Investigative Dermatology* **114**, 533–540.
- STÜCKER, M., FALKENBERG, M., REUTHER, T., ALTMAYER, P. & LÜBBERS, D. W. (2000b). Local oxygen content in the skin is increased in chronic venous incompetence. *Microvascular Research* **59**, 99–106.
- VAUPEL, P. (1976). Effect of percental water content in tissue and liquids on the diffusion coefficients of O₂, CO₂, N₂, H₂. *Pflügers Archiv* **361**, 201–204.
- WADE, O. L. & BISHOP, J. M. (1962). *Cardiac Output and Regional Blood Flow*. Blackwell, Oxford.
- WILSON, D. F., ERECINSKA, M., DROWN, C. & SILVER, I. A. (1979). The oxygen dependence of cellular energy metabolism. *Archives of Biochemistry and Biophysics* **195**, 485–493.
- YAAR, M. & GILCHREST, B. A. (1999). Aging of skin. In *Fitzpatrick's Dermatology in General Medicine*, 5th edn, ed. FREEDBERG, I. M., EISEN, A. Z., WOLFF, K., AUSTEN, K. F., GOLDSMITH, L. A., KATZ, S. I. & FITZPATRICK, T. B., pp. 1697–1706. McGraw-Hill, New York.

Acknowledgements

We wish to thank Courage and Khazaka GmbH, Cologne, Germany for providing the corneometer SM 825 PC, D. Seiler (Max-Planck-Institute) for the fabrication of the platinum electrode, S. Mischke (Max-Planck-Institute) for proof reading the manuscript and D. Pieck (Department of Dermatology) for assistance during the experiments. This work was supported by a grant from the Deutsche Forschungsgemeinschaft (DFG, Al 389/4-1 and 4-2).